

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**            **KR 109**  
**Lot Number**                **8203**

**Date**            08.10.2008


**Expiry Date**            08.10.2009

Reagent	Lot Number
AMM 1	8029
<b>Amm 2</b>	<b>8203</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.024
0.25	AMM 10 09 08	0.227
0.50	AMM 10 09 08	0.438
0.77	AMM 10 09 08	0.665
1.00	AMM 10 09 08	0.861


*\*serial dilution*

#### Calibration Curve

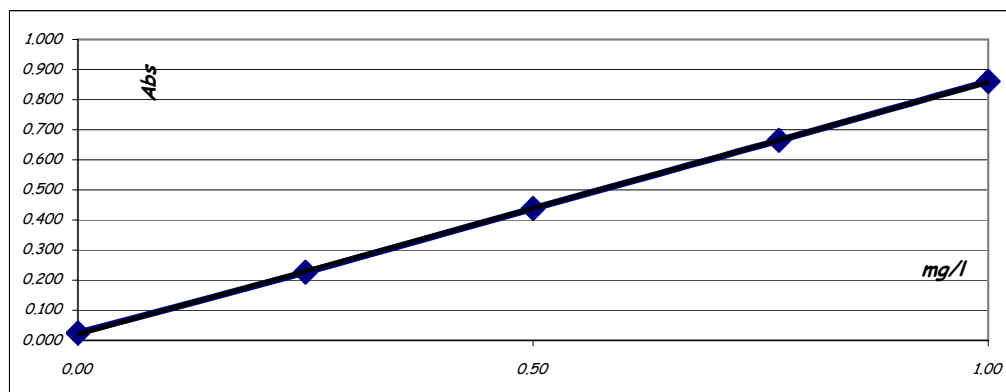

Test	Result	Specification	Pass / Fail
Intercept	0.0206	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8381	0.750 to 0.890	<b>Pass</b>
Regression	0.9999	0.990 to 1.0001	<b>Pass</b>

**Notes**    *Store between 2 & 8 °c*  
*\*Stable on Board 5 days*  
*Barcode ID = 109*  
*\* Based on results obtained in our Research Facility*


---

 Dr. T. Russell