

Certificate of Performance

Nitrite Reagent

Product Code KR105
Lot Number 9027

Date 28.01.2009


Expiry Date 02.01.2010

Reagent	Lot Number
TON3	9027
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0.00		0.000
0.50	NO2-20 10 08	0.417
1.00	NO2-20 10 08	0.818
1.54	NO2-20 10 08	1.273
2.00	NO2-20 10 08	1.693

*serial dilution

Calibration Curve

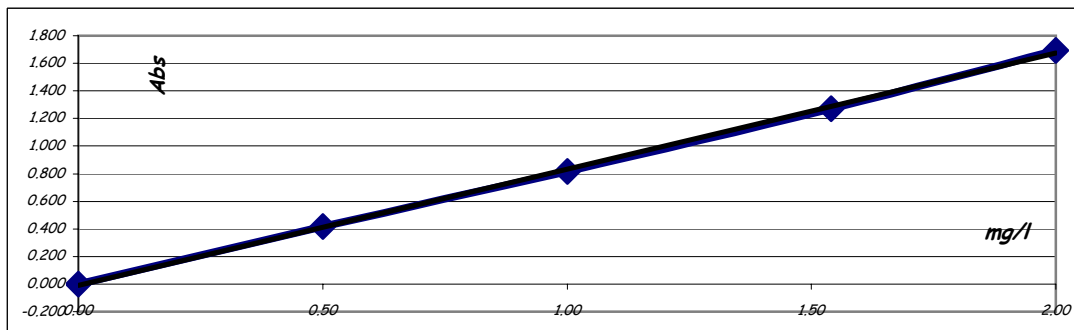

Test	Result	Specification	Pass / Fail
Intercept	-0.008	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.841	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °c
**Stable on Board 5 days*
Barcode ID = 105
** Based on results obtained in our Research Facility*



Dr. T. Russell