Precision®

'Ready To Use Reagents'

version 2006.01

Certificate of Performance

Nitrite Reagent

Product Code KR105

Lot Number 9040

Date 12.02.2009 **Expiry Date** 12.02.2010

Reagent	Lot Number
TON3	9040
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0.00		0.000
0.50	NO2-20 10 08	0.435
1.00	NO2-20 10 08	0.862
1.54	NO2-20 10 08	1.325
2.00	NO2-20 10 08	1.729

*serial dilution

Calibration Curve

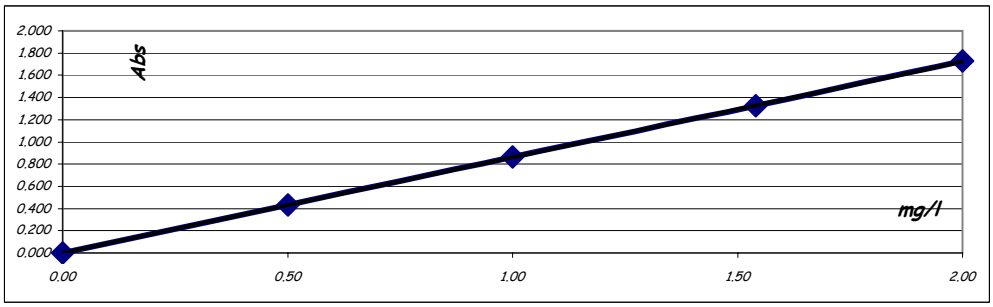

Test	Result	Specification			Pass / Fail
Intercept	0.001	-0.010	to	0.010	Pass
Sensitivity Abs/ppm	0.863	0.750	to	0.900	Pass
Regression	1.000	0.990	to	1.001	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 105
** Based on results obtained in our Research Facility*

Tom Russell

Dr. T. Russell

Serosep

An ISO 9001:2000 Registered Company

Unit F5, Eastway Business Park, Ballysimon Road, Limerick, Ireland.

Telephone 061 440207 Facsimile 061 440237