

**Certificate of Performance**

**Chloride Reagent**

**Product Code** KR101  
**Lot Number** 9142


**Date** 14.08.2009 **Expiry Date** 22.07.2010

<b>Reagent</b>	<b>Lot Number</b>
Chloride	9142
<b>Test Method</b>	LTP02
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.001
250 ppm	CL4000 03 09	0.266
500 ppm	CL4000 03 09	0.416
800 ppm	CL4000 03 09	0.539
1000 ppm	CL4000 03 09	0.611

\*serial Dilution

**Calibration Curve**

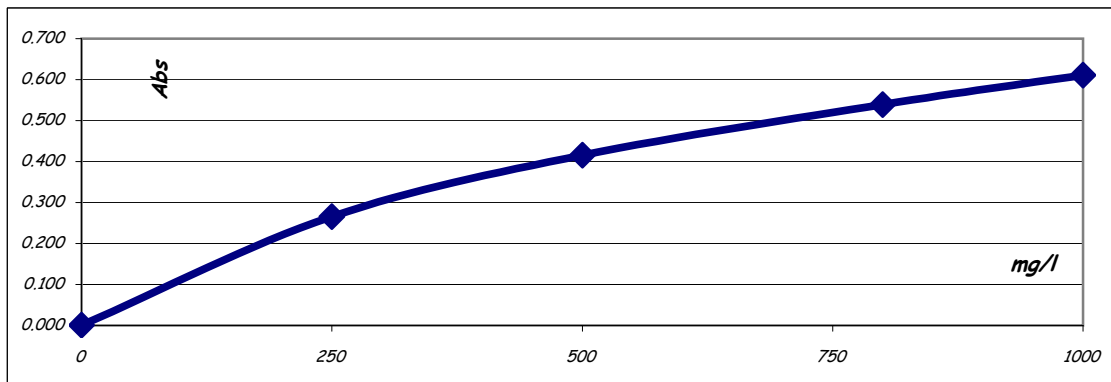

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0011	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0006	0.0006 to 0.0012	Pass
500 - 800 mg/l	0.0004	0.0004 to 0.0010	Pass
800 - 1000 mg/l	0.0004	0.0003 to 0.0008	Pass

**Notes** Store between 2 & 8 °c  
 \*Stable on Board 5 days  
 Barcode ID = 101  
 \* Based on results obtained in our Research Facility

*Tom Russell*

Dr. T. Russell