

Certificate of Performance
Sulphate Reagent

Product Code KR102
Lot Number 9165

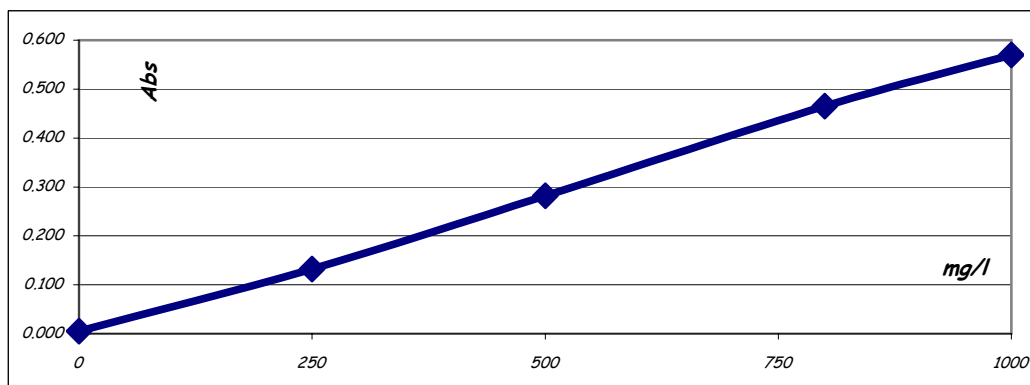
Date 04.09.2009

Expiry Date 01.09.2010

Reagent	Lot Number
Sulphate	9165
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.005
250	Sulp 4000 07 09	0.132
500	Sulp 4000 07 09	0.282
800	Sulp 4000 07 09	0.465
1000	Sulp 4000 07 09	0.570

*serial Dilution

Calibration Curve


Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.010	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0005	0.0003 to 0.0006	Pass
250 - 500 mg/l	0.0006	0.0003 to 0.0007	Pass
500 - 800 mg/l	0.0006	0.0004 to 0.0007	Pass
800 - 1000 mg/l	0.0005	0.0004 to 0.0008	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 102
 * Based on results obtained in our Research Facility



Dr. T. Russell

An ISO 9001:2000 Registered Company