

### Certificate of Performance

#### Ammonia 1 Reagent

**Product Code**            **KR108**  
**Lot Number**                **9179**

**Date**            29.09.2009


**Expiry Date**            28.09.2010

Reagent	Lot Number
AMM 1	<b>9179</b>
Amm 2	9120
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.028
0.25	AMM 10 04 09	0.224
0.50	AMM 10 04 09	0.434
0.77	AMM 10 04 09	0.660
1.00	AMM 10 04 09	0.856

*\*serial dilution*

#### Calibration Curve

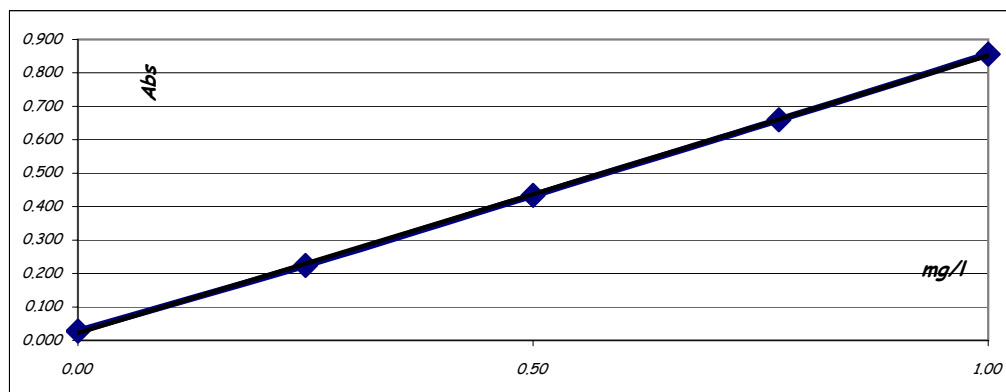

Test	Result	Specification	Pass / Fail
Intercept	0.0220	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8301	0.750 to 0.890	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

*Notes*    *Store between 2 & 8 °c*  
*\*Stable on Board 1 day*  
*Barcode ID = 108*  
*\* Based on results obtained in our Research Facility*


---

*Dr. T. Russell*