

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **9191**

Date 22.10.2009


Expiry Date 21.10.2010

Reagent	Lot Number
AMM 1	9121
Amn 2	9191
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.021
0.25	AMM 10 10 09	0.226
0.50	AMM 10 10 09	0.440
0.77	AMM 10 10 09	0.671
1.00	AMM 10 10 09	0.870


**serial dilution*

Calibration Curve

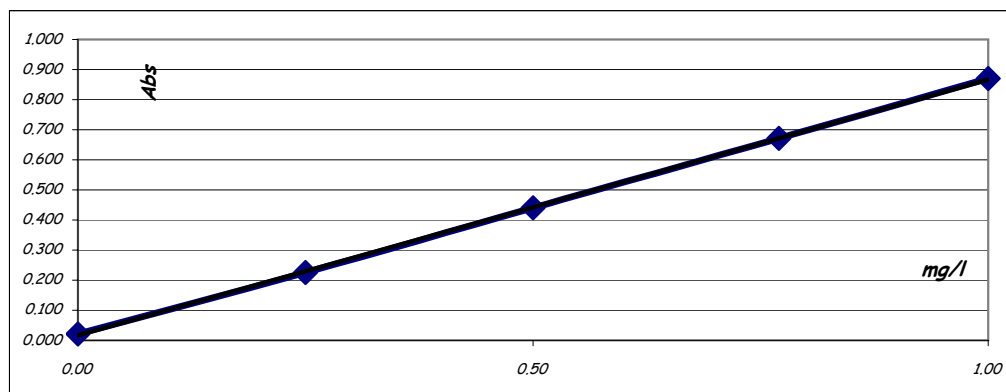

Test	Result	Specification	Pass / Fail
Intercept	0.0170	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8504	0.750 to 0.890	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*
 **Stable on Board 5 days*
 Barcode ID = 109
 ** Based on results obtained in our Research Facility*



 Dr. T. Russell