Precision®

Ready To Use Reagents' Ver 2006:03

Certificate of Performance

TON 3

Product Code KR105

Date 14.04.2010 **Expiry Date** 22.03.2011

Reagent	Lot Number
TON 1	0021
TON 2	9141
TON 3	**0080**
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.005
2.50	TON 100 02 10	0.200
5.00	TON 100 02 10	0.373
7.69	TON 100 02 10	0.563
10.00	TON 100 02 10	0.688

*serial dilution

Calibration Curve

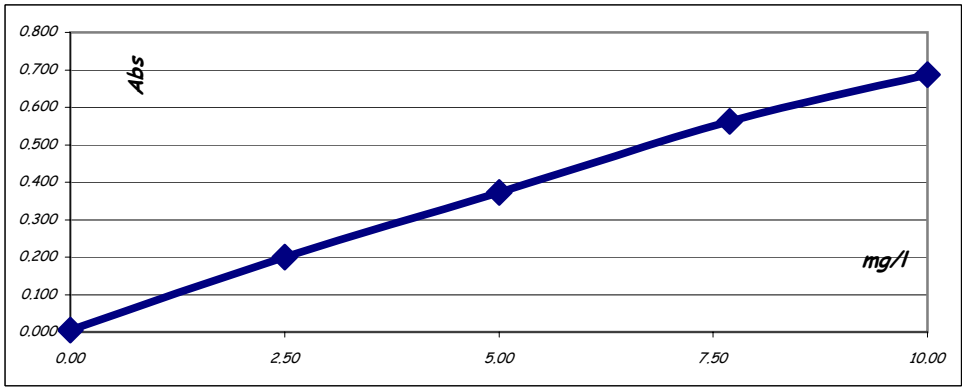

Test		Result	Specification			Pass / Fail
Intercept		0.005	-0.005	to	0.01	**Pass**
Sensitivity	Abs/ppm					
	0 - 2.50 mg/l	0.0780	0.0550	to	0.0800	**Pass**
	2.50 - 5.00 mg/l	0.0692	0.0600	to	0.0800	**Pass**
	5.00 - 7.69 mg/l	0.0706	0.0550	to	0.0800	**Pass**
	7.69 - 10.0 mg/l	0.0541	0.0500	to	0.0700	**Pass**

Notes *Store between 2 & 8 °C*

**Stable on Board TON 1 - 1 day*

** TON 2 & TON 3 - 5 days*

Keep Tightly Sealed when not in use.

Do not return unused portions to container

Barcode ID- TON 1 103; TON 2 104; TON 3 105

** Based on results obtained in our Research Facility*

Tom Russell.

Dr. T. Russell

Serosep laboratory diagnostics

An ISO 9001:2000 Registered Company

Unit F5, Eastway Business Park, Ballysimon Road, Limerick, Ireland.

Telephone 061 440207 Facsimile 061 440237