

Certificate of Performance

Silica 3

Product Code KR116
Lot Number 0085

Date 20.05.2010


Expiry Date 16.02.2011

Reagent	Lot Number
Silica 1	0083
Silica 2	0084
Silica 3	0085
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0.00	Silica-200 03 10	0.001
5.00	Silica-200 03 10	0.394
10.00	Silica-200 03 10	0.763
15.39	Silica-200 03 10	1.190
20.00	Silica-200 03 10	1.536

*serial dilution

Calibration Curve

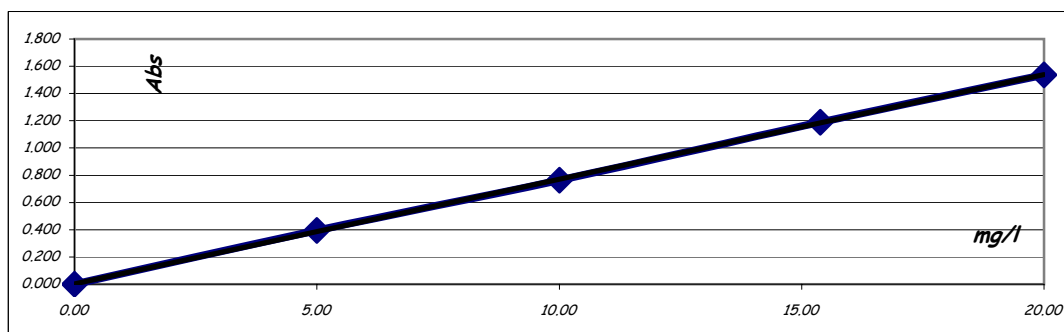

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.767	0.700 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °c
 *Stable on Board 5 days
 Barcode ID = 116
 * Based on results obtained in our Research Facility



Dr. T. Russell