

Certificate of Performance

Alkalinity 2 Reagent

Product Code **KR112**

Lot Number **0095**

Date **28.04.2010**


Expiry Date **28.10.2010**

Reagent	Lot Number
Alkalinity 2	0095
Test Method	LTP08
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.003
100	Alkal 4000 04 10	0.630
200	Alkal 4000 04 10	1.085
307.7	Alkal 4000 04 10	1.378
400	Alkal 4000 04 10	1.513

*serial Dilution

Calibration Curve

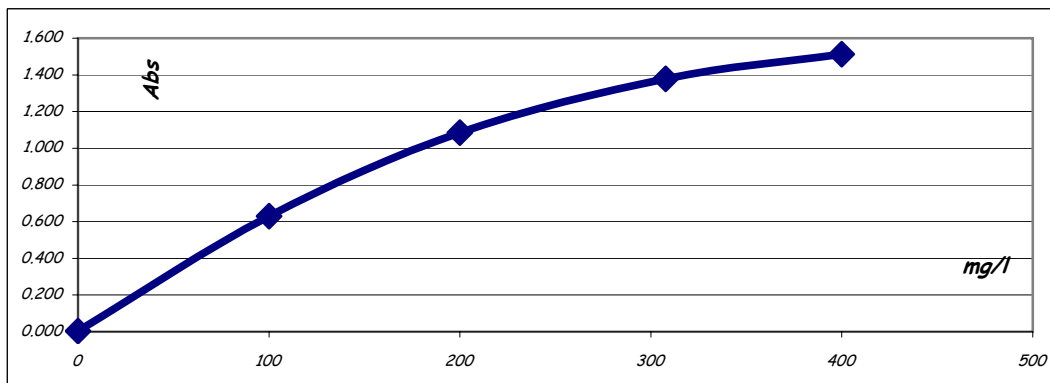

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.090	Pass
Sensitivity	Abs/ppm		
	0 - 100 mg/l	0.0063 to 0.0090	Pass
	100 - 200 mg/l	0.0046 to 0.0080	Pass
	200 - 307.7 mg/l	0.0027 to 0.0050	Pass
	307.7 - 400 mg/l	0.0015 to 0.0040	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 112
** Based on results obtained in our Research Facility*



Dr. T. Russell

An ISO 9001:2000 Registered Company

Unit F5, Eastway Business Park, Ballysimon Road, Limerick, Ireland.

Telephone 061 440207

Facsimile 061 440237