



*'Ready To Use Reagents'*

**Certificate of Performance**

**Phosphate 1 (Phos 1) Reagent**

**Product Code** KR106  
**Lot Number** 0107

**Date** 25.05.2010


**Expiry Date** 17.05.2011

Reagent	Lot Number
Phos 1	0107
Phos 2	9228
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P20 01 10	0.152
1	P20 01 10	0.294
1.5	P20 01 10	0.452
2	P20 01 10	0.575

\*serial dilution

**Calibration Curve**

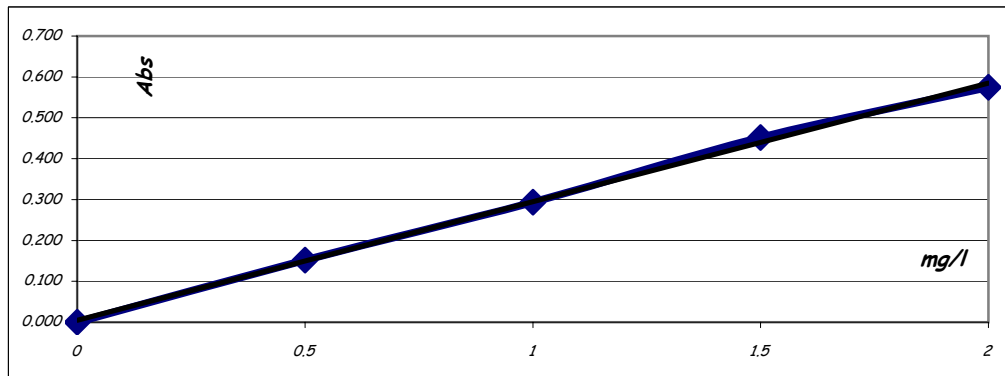

	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.010	<b>Pass</b>
Sensitivity Abs/ppm	0.290	0.260 to 0.320	<b>Pass</b>
Regression	0.999	0.990 to 1.001	<b>Pass</b>

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 106  
 \* Based on results obtained in our Research Facility

*Dr. T. Russell*



An ISO 9001:2000 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.

Telephone 061 358190

Facsimile 061 358191