

Certificate of Performance

Ammonia 1 Reagent

Product Code **KR108**
Lot Number **0194**

Date 13.10.2010


Expiry Date 12.10.2011

Reagent	Lot Number
AMM 1	0194
Amm 2	0193
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.020
0.25	AMM 10 08 10	0.229
0.50	AMM 10 08 10	0.434
0.77	AMM 10 08 10	0.663
1.00	AMM 10 08 10	0.852

**serial dilution*

Calibration Curve

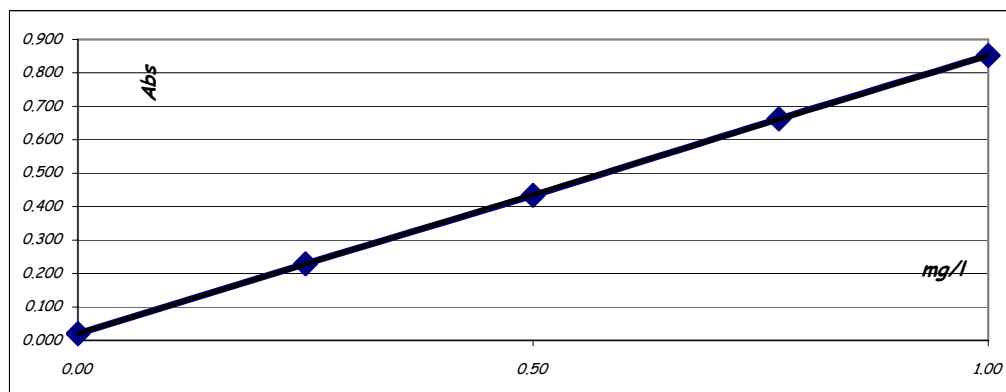

Test	Result	Specification	Pass / Fail
Intercept	0.0200	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8326	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*
 **Stable on Board 1 day*
 Barcode ID = 108
 ** Based on results obtained in our Research Facility*



 Dr. T. Russell