



*'Ready To Use Reagents'*

**Certificate of Performance**

**Phosphate 2 (Phos 2) Reagent**

**Product Code** KR107  
**Lot Number** 0195

**Date** 13.10.2010


**Expiry Date** 23.09.2011

Reagent	Lot Number
Phos 1	0025
Phos 2	0195
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 09 10	0.145
1	P20 09 10	0.289
1.5	P20 09 10	0.439
2	P20 09 10	0.573

\*serial dilution

**Calibration Curve**

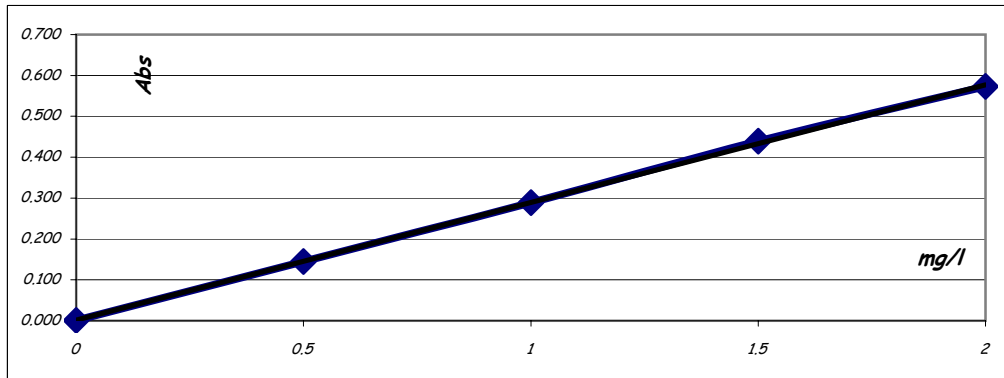

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.288	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

*Tom Russell.*  
 \_\_\_\_\_  
 Dr. T. Russell



An ISO 9001:2000 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.  
 Telephone 061 358190 Facsimile 061 358191