



*'Ready To Use Reagents'*

**Certificate of Performance**

**Phosphate 1 (Phos 1) Reagent**

**Product Code** KR106

**Lot Number** 0208

**Date** 02.11.2010


**Expiry Date** 01.11.2011

Reagent	Lot Number
Phos 1	0208
Phos 2	0195
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P20 06 10	0.150
1	P20 06 10	0.301
1.5	P20 06 10	0.445
2	P20 06 10	0.585

\*serial dilution

**Calibration Curve**

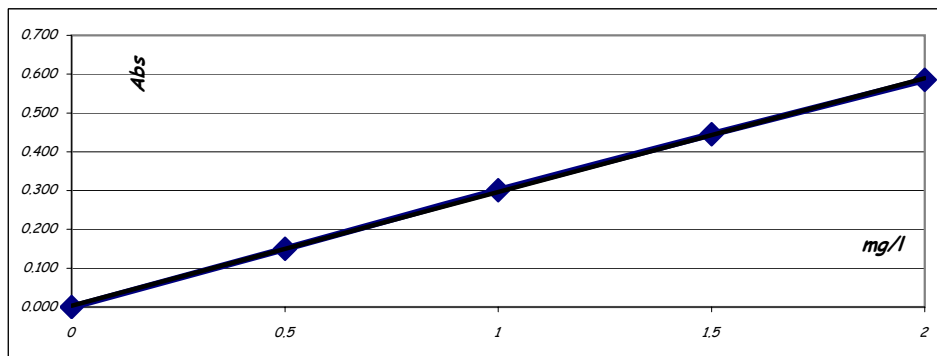

	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.293	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 106  
 \* Based on results obtained in our Research Facility

*Dr. T. Russell*

An ISO 9001:2008 Registered Company

Annacotty Business Park, Annacotty, Limerick

Telephone 061 358190

Facsimile 061 358191

