

Certificate of Performance

Alkalinity 2 Reagent

Product Code **KR112**

Lot Number **0225**

Date **12.11.2010**


Expiry Date **11.09.2011**

Reagent	Lot Number
Alkalinity 2	0225
Test Method	LTP08
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.040
100	Alkal 4000 11 10	0.592
200	Alkal 4000 11 10	1.008
307.7	Alkal 4000 11 10	1.283
400	Alkal 4000 11 10	1.440

*serial Dilution

Calibration Curve

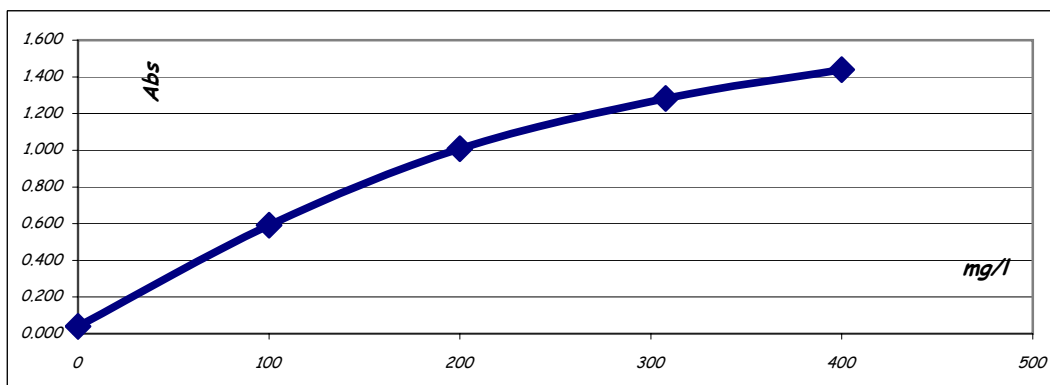

Test	Result	Specification	Pass / Fail
Intercept	0.040	-0.005 to 0.090	Pass
Sensitivity	Abs/ppm		
	0 - 100 mg/l	0.0055 to 0.0090	Pass
	100 - 200 mg/l	0.0042 to 0.0080	Pass
	200 - 307.7 mg/l	0.0026 to 0.0050	Pass
	307.7 - 400 mg/l	0.0017 to 0.0040	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 112
** Based on results obtained in our Research Facility*



Dr. T. Russell

An ISO 9001:2000 Registered Company

Unit F5, Eastway Business Park, Ballysimon Road, Limerick, Ireland.

Telephone 061 440207

Facsimile 061 440237