

Certificate of Performance

Ammonia 1 Reagent

Product Code KR108
Lot Number 0276

Date 21.12.2010


Expiry Date 01.12.2011

Reagent	Lot Number
AMM 1	0276
Amm 2	0277
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.023
0.25	AMM 10 07 10	0.225
0.50	AMM 10 07 10	0.418
0.77	AMM 10 07 10	0.646
1.00	AMM 10 07 10	0.835

**serial dilution*

Calibration Curve

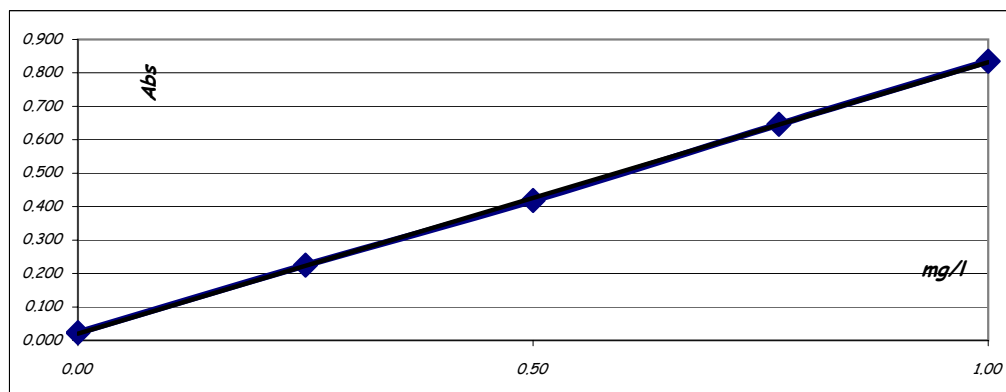

Test	Result	Specification	Pass / Fail
Intercept	0.0204	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8115	0.750 to 0.890	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*
 **Stable on Board 1 day*
 Barcode ID = 108
 ** Based on results obtained in our Research Facility*



 Dr. T. Russell