Precision®

'Ready To Use Reagents' ver 2009.02

Certificate of Performance

Sulphate Reagent

Product Code KR102

Lot Number 1012

Date 28.01.2011 **Expiry Date** 18.01.2012

Reagent	Lot Number
Sulphate	1012
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.006
250	Sulp 4000 05 10	0.115
500	Sulp 4000 05 10	0.243
800	Sulp 4000 05 10	0.399
1000	Sulp 4000 05 10	0.490

*serial Dilution

Calibration Curve

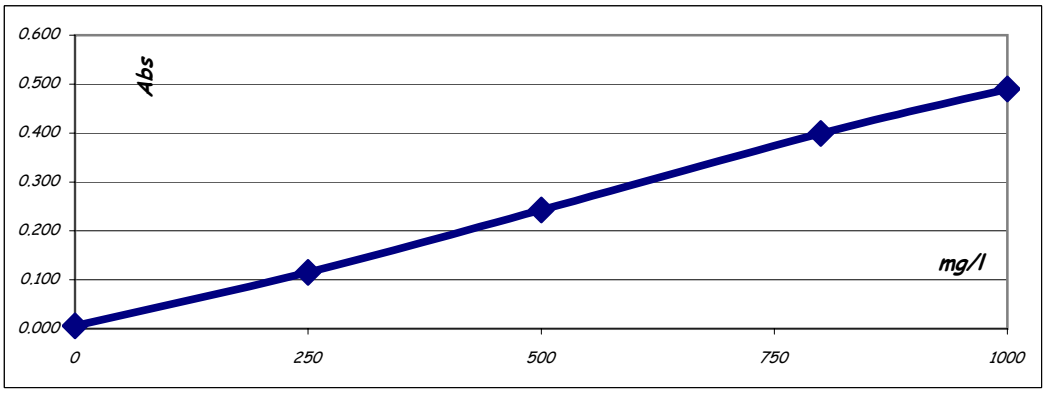

Test		Result	Specification			Pass / Fail
Intercept		0.006	-0.005	to	0.010	Pass
Sensitivity	Abs/ppm					
	0 - 250 mg/l	0.0004	0.0003	to	0.0006	Pass
	250 - 500 mg/l	0.0005	0.0003	to	0.0007	Pass
	500 - 800 mg/l	0.0005	0.0004	to	0.0007	Pass
	800 - 1000 mg/l	0.0005	0.0004	to	0.0008	Pass

Notes *Store between 2 & 8 °C*
**Stable on Board 5 days*
Barcode ID = 102
** Based on results obtained in our Research Facility*

Tom Russell.

Dr. T. Russell

Serosep

An ISO 9001:2000 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.

Telephone 061 358190 Facsimile 061 358191