

Certificate of Performance

Nitrite Reagent

Product Code **KR105**
Lot Number **1027**

Date 01.02.2011


Expiry Date 31.01.2012

Reagent	Lot Number
TON3	1027
Test Method	LTP04
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0.00		0.001
0.50	NO2-20 06 10	0.432
1.00	NO2-20 06 10	0.843
1.54	NO2-20 06 10	1.298
2.00	NO2-20 06 10	1.670

*serial dilution

Calibration Curve

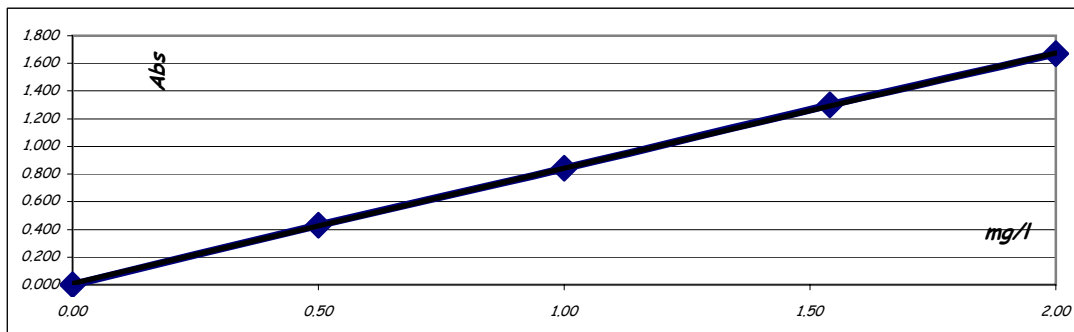

Test	Result	Specification	Pass / Fail
Intercept	0.008	-0.010 to 0.010	Pass
Sensitivity Abs/ppm	0.834	0.750 to 0.900	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 105
** Based on results obtained in our Research Facility*



Dr. T. Russell