

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      KR 109  
**Lot Number**        1042

**Date**      25.02.2011


**Expiry Date**      24.01.2012

Reagent	Lot Number
AMM 1	1041
<b>Amn 2</b>	<b>1042</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.029
0.25	AMM 10 02 11	0.222
0.50	AMM 10 02 11	0.428
0.77	AMM 10 02 11	0.645
1.00	AMM 10 02 11	0.846

*\*serial dilution*

#### Calibration Curve

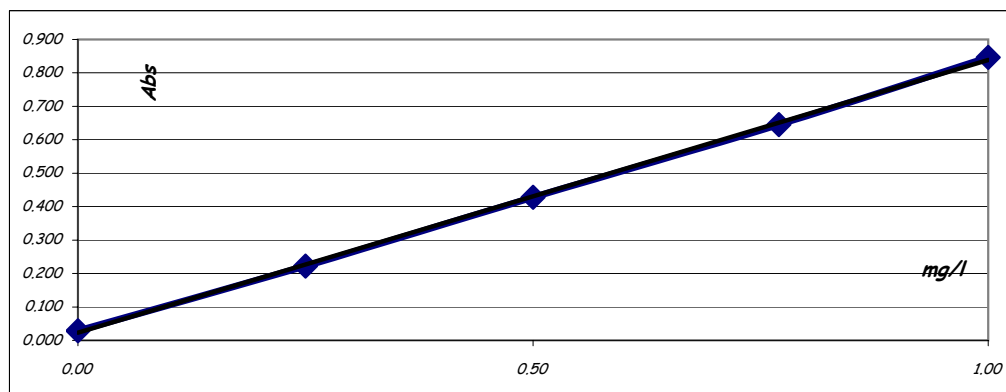

Test	Result	Specification	Pass / Fail
Intercept	0.0227	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8161	0.750 to 0.890	<b>Pass</b>
Regression	0.9996	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °c*  
                  *\*Stable on Board 5 days*  
                  *Barcode ID = 109*  
                  *\* Based on results obtained in our Research Facility*


---

 Dr. T. Russell