

Certificate of Performance
Hard 3

Product Code KR119

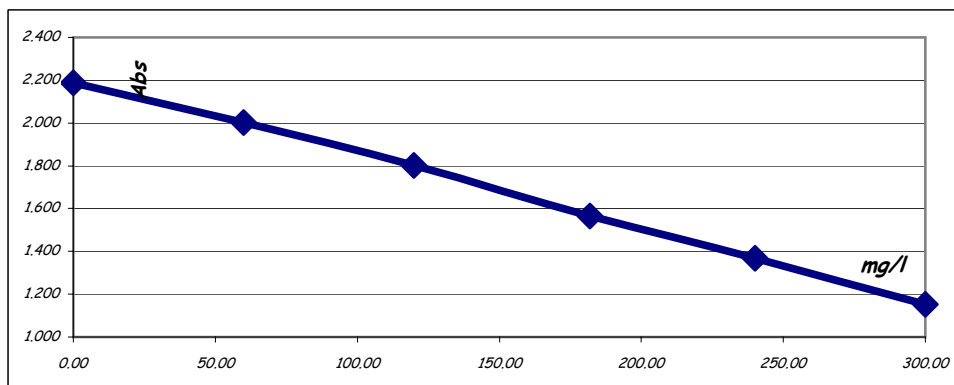
Date 04.03.2011

Expiry Date 01.03.2012

Reagent	Lot Number
Hard 1	1060
Hard 2	1061
Hard 3	1062
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00	Hard3000 02 11	2.187
60.00	Hard3000 02 11	2.002
120.00	Hard3000 02 11	1.802
181.82	Hard3000 02 11	1.566
240.00	Hard3000 02 11	1.369
300.00	Hard3000 02 11	1.152

*serial dilution

Calibration Curve


Test	Result	Pass / Fail
0	2.534	Pass
60	2.381	Pass
120	2.154	Pass
181.8182	1.928	Pass
240	1.69	Pass
300	1.476	Pass

Notes Store between 2 & 8 °C

Keep Tightly Sealed when not in use.

Do not return unused portions to container

Barcode ID- Hard 1 117; Hard 2 118; Hard 3 119

* Based on results obtained in our Research Facility



Dr. T. Russell