

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      KR 109  
**Lot Number**        1076

**Date**      24.03.2011


**Expiry Date**      11.03.2012

Reagent	Lot Number
AMM 1	1041
<b>Amm 2</b>	<b>1076</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.027
0.25	AMM 10 02 11	0.216
0.50	AMM 10 02 11	0.415
0.77	AMM 10 02 11	0.632
1.00	AMM 10 02 11	0.827


*\*serial dilution*

#### Calibration Curve

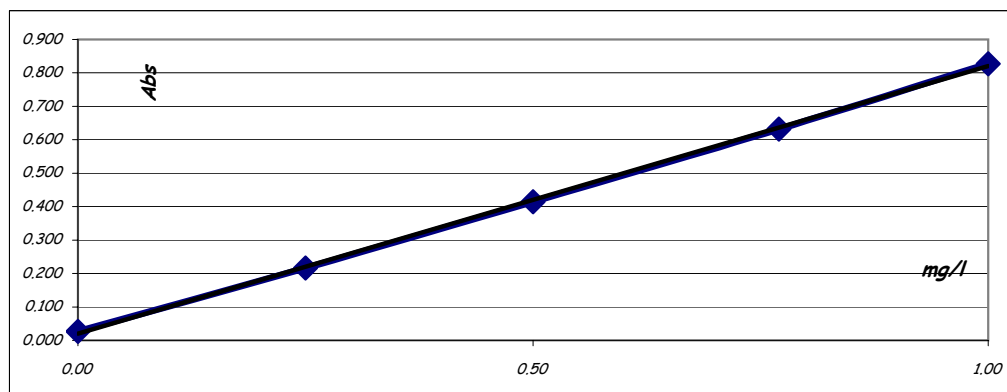

Test	Result	Specification	Pass / Fail
Intercept	0.0203	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.7999	0.750 to 0.890	<b>Pass</b>
Regression	0.9996	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °c*  
               *\*Stable on Board 5 days*  
               *Barcode ID = 109*  
               *\* Based on results obtained in our Research Facility*


---

 Dr. T. Russell