

Certificate of Performance

Hard 3

Product Code KR119

Date 28.03.2011


Expiry Date 22.02.2012

| Reagent | Lot Number |
|-----------------|------------|
| Hard 1 | 1060 |
| Hard 2 | 1061 |
| Hard 3 | 1081 |
| Test Instrument | Konelab 20 |
| Serial Number | P4919028 |

| Std. Value | Lot # | Abs. |
|------------|-----------------|-------|
| 0.00 | Hard 3000 02 11 | 2.298 |
| 60.00 | Hard 3000 02 11 | 2.142 |
| 120.00 | Hard 3000 02 11 | 1.944 |
| 181.82 | Hard 3000 02 11 | 1.714 |
| 240.00 | Hard 3000 02 11 | 1.481 |
| 300.00 | Hard 3000 02 11 | 1.283 |

*serial dilution

Calibration Curve

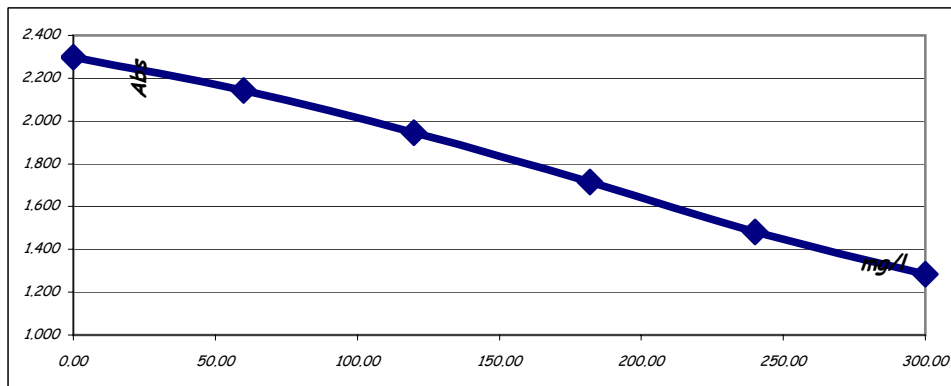

| Test | Result | Specification | Pass / Fail |
|-------------------|---------|--------------------|-------------|
| Sensitivity | | | |
| 0 - 60 mg/l | -0.0026 | -0.0025 to -0.0035 | Pass |
| 60 - 120 mg/l | -0.0033 | -0.0030 to -0.0045 | Pass |
| 120 - 181.82 mg/l | -0.0038 | -0.0035 to -0.0045 | Pass |
| 181.82 - 240 mg/l | -0.0039 | -0.0030 to -0.0040 | Pass |
| 240 - 300 mg/l | -0.0033 | -0.0025 to -0.0040 | Pass |

Notes Store between 2 & 8 °C

Keep Tightly Sealed when not in use.

Do not return unused portions to container

Barcode ID- Hard 1 117; Hard 2 118; Hard 3 119

* Based on results obtained in our Research Facility



Dr. T. Russell