

Certificate of Performance
TON 1

Product Code KR103

Date 30.03.2011

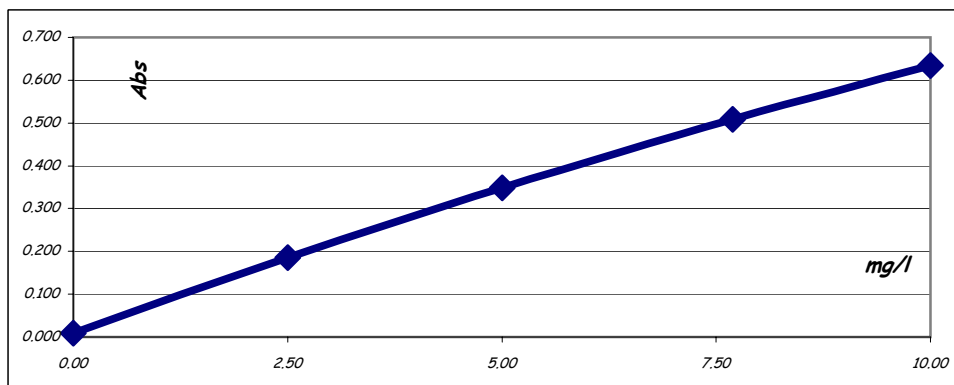
Expiry Date

30.03.2012

Reagent	Lot Number
TON 1	1084
TON 2	1077
TON 3	1082
Test Method	LMTP03
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.009
2.50	TON 100 03 11	0.185
5.00	TON 100 03 11	0.348
7.69	TON 100 03 11	0.509
10.00	TON 100 03 11	0.634

*serial dilution

Calibration Curve


Test	Result	Specification	Pass / Fail
Intercept	0.009	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.50 mg/l	0.0704	0.0550 to 0.0800	Pass
2.50 - 5.00 mg/l	0.0652	0.0600 to 0.0800	Pass
5.00 - 7.69 mg/l	0.0599	0.0550 to 0.0800	Pass
7.69 - 10.0 mg/l	0.0541	0.0500 to 0.0700	Pass

Notes

Store between 2 & 8 °C

*Stable on Board TON 1 - 1 day

* TON 2 & TON 3 - 5 days

Keep Tightly Sealed when not in use.

Do not return unused portions to container

Barcode ID- TON 1 103; TON 2 104; TON 3 105

* Based on results obtained in our Research Facility



Dr. T. Russell