



*'Ready To Use Reagents'*

**Certificate of Performance**

**Phosphate 1 (Phos 1) Reagent**

**Product Code** KR106  
**Lot Number** 1085

**Date** 31.03.2011


**Expiry Date** 05.01.2012

Reagent	Lot Number
Phos 1	1085
Phos 2	0195
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P20 02 11	0.149
1	P20 02 11	0.297
1.5	P20 02 11	0.454
2	P20 02 11	0.587

\*serial dilution

**Calibration Curve**

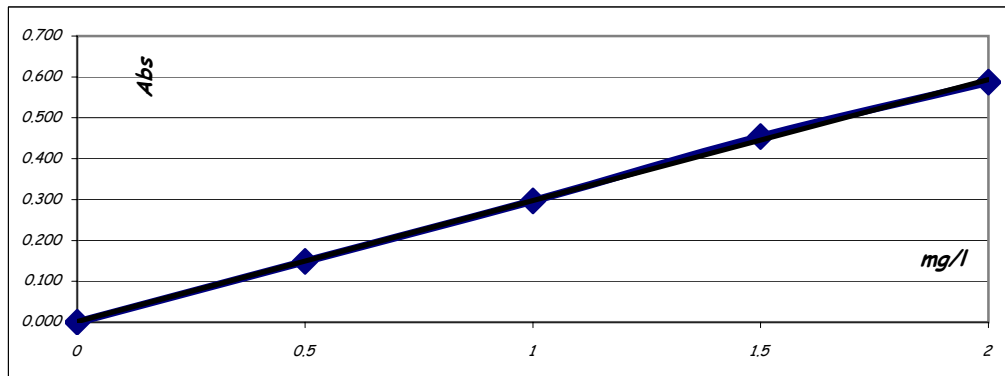

	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.296	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 106  
 \* Based on results obtained in our Research Facility

*Dr. T. Russell*



An ISO 9001:2008 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.

Telephone 061 358190

Facsimile 061 358191