

Certificate of Performance

Ammonia 1 Reagent

Product Code **KR108**
Lot Number **1113**

Date 29.04.2011


Expiry Date 26.04.2012

Reagent	Lot Number
AMM 1	1113
Amm 2	0159
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.028
0.25	AMM 10 04 11	0.215
0.50	AMM 10 04 11	0.427
0.77	AMM 10 04 11	0.651
1.00	AMM 10 04 11	0.828

**serial dilution*

Calibration Curve

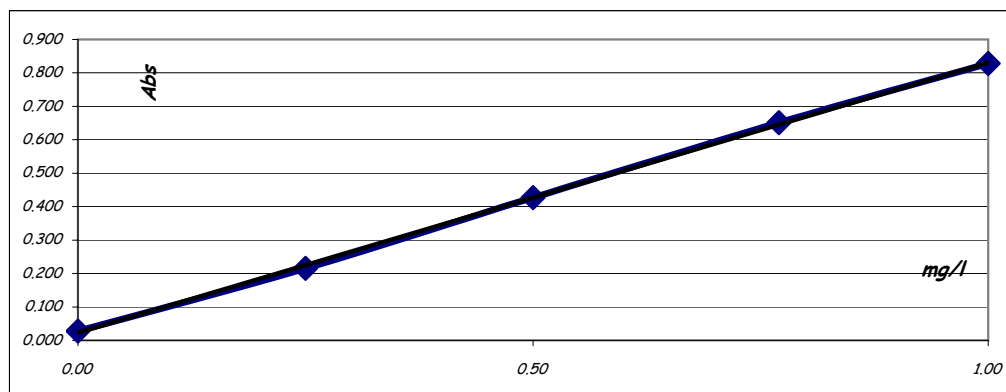

Test	Result	Specification	Pass / Fail
Intercept	0.0225	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8081	0.750 to 0.890	Pass
Regression	0.9996	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*

**Stable on Board 1 day*

Barcode ID = 108

** Based on results obtained in our Research Facility*



Dr. T. Russell