



'Ready To Use Reagents'

version 2011.01

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107
Lot Number 1115

Date 29.04.2011


Expiry Date 01.03.2012

Reagent	Lot Number
Phos 1	1071
Phos 2	1115
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P20 02 11	0.156
1	P20 02 11	0.299
1.5	P20 02 11	0.458
2	P20 02 11	0.588

*serial dilution

Calibration Curve

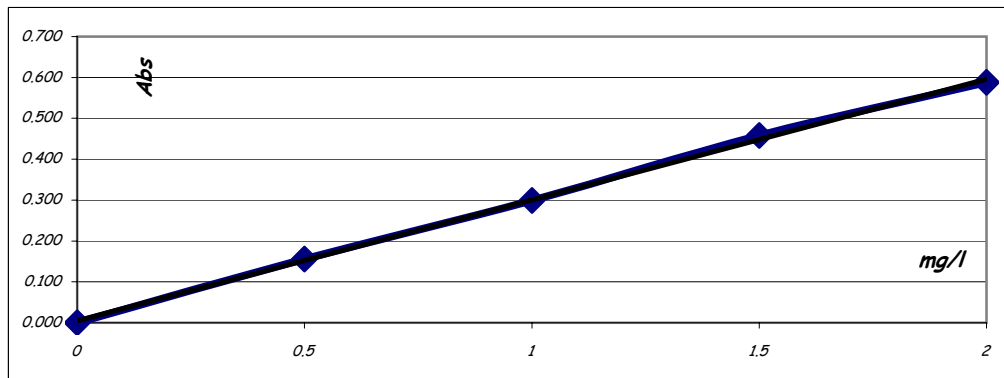

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.296	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 107
 * Based on results obtained in our Research Facility

Tom Russell.
 Dr. T. Russell



An ISO 9001:2008 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.
 Telephone 061 358190 Facsimile 061 358191