



'Ready To Use Reagents'

version 2011.01

### Certificate of Performance

## Phosphate 2 (Phos 2) Reagent

Product Code KR107  
Lot Number 1126

Date 10.05.2011


Expiry Date 11.03.2012

Reagent	Lot Number
Phos 1	1125
Phos 2	1126
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 02 11	0.160
1	P20 02 11	0.310
1.5	P20 02 11	0.465
2	P20 02 11	0.607

\*serial dilution

### Calibration Curve

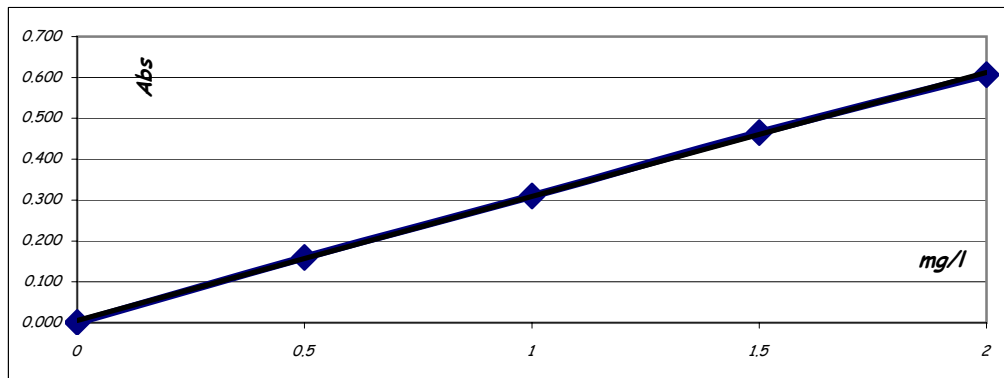

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.303	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

Dr. T. Russell



An ISO 9001:2008 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.

Telephone 061 358190

Facsimile 061 358191