

Certificate of Performance

Chloride Reagent

Product Code KR101
Lot Number 1161


Date 21.06.2011 **Expiry Date** 19.05.2012

Reagent	Lot Number
Chloride	1161
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.004
250 ppm	CL4000 08 10	0.317
500 ppm	CL4000 08 10	0.517
800 ppm	CL4000 08 10	0.675
1000 ppm	CL4000 08 10	0.758

*serial Dilution

Calibration Curve

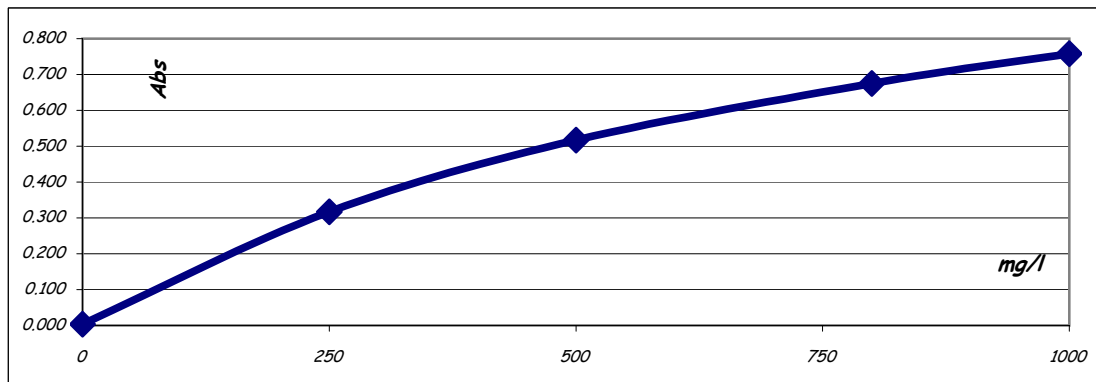

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0013	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0008	0.0006 to 0.0012	Pass
500 - 800 mg/l	0.0005	0.0004 to 0.0010	Pass
800 - 1000 mg/l	0.0004	0.0003 to 0.0008	Pass

Notes Store between 2 & 8 °c
 *Stable on Board 5 days
 Barcode ID = 101
 * Based on results obtained in our Research Facility

Tom Russell

Dr. T. Russell