

### Certificate of Performance

#### Ammonia 1 Reagent

**Product Code**            **KR108**  
**Lot Number**                **1169**

**Date**            29.07.2011


**Expiry Date**            29.06.2012

Reagent	Lot Number
AMM 1	<b>1169</b>
Amm 2	1042
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.024
0.25	AMM 10 07 11	0.224
0.50	AMM 10 07 11	0.430
0.77	AMM 10 07 11	0.654
1.00	AMM 10 07 11	0.853

*\*serial dilution*

#### Calibration Curve

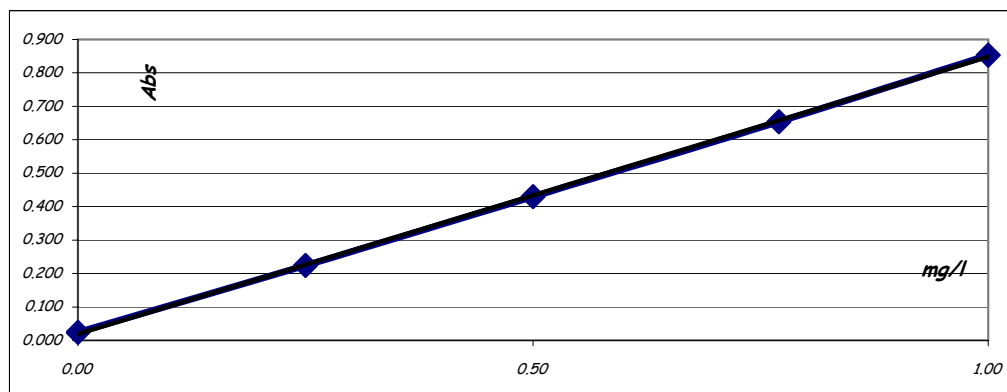

Test	Result	Specification	Pass / Fail
Intercept	0.0195	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8285	0.750 to 0.890	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

*Notes*    *Store between 2 & 8 °c*

*\*Stable on Board 1 day*

*Barcode ID = 108*

*\* Based on results obtained in our Research Facility*



*Dr. T. Russell*