



'Ready To Use Reagents'

version 2011.01

**Certificate of Performance**

**Phosphate 2 (Phos 2) Reagent**

**Product Code** KR107  
**Lot Number** 1172

**Date** 05.07.2011


**Expiry Date** 05.07.2012

Reagent	Lot Number
Phos 1	1071
Phos 2	1172
<b>Test Method</b>	LTP 05
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Abs.
0		0.001
0.5	P20 02 11	0.148
1	P20 02 11	0.300
1.5	P20 02 11	0.465
2	P20 02 11	0.592

\*serial dilution

**Calibration Curve**

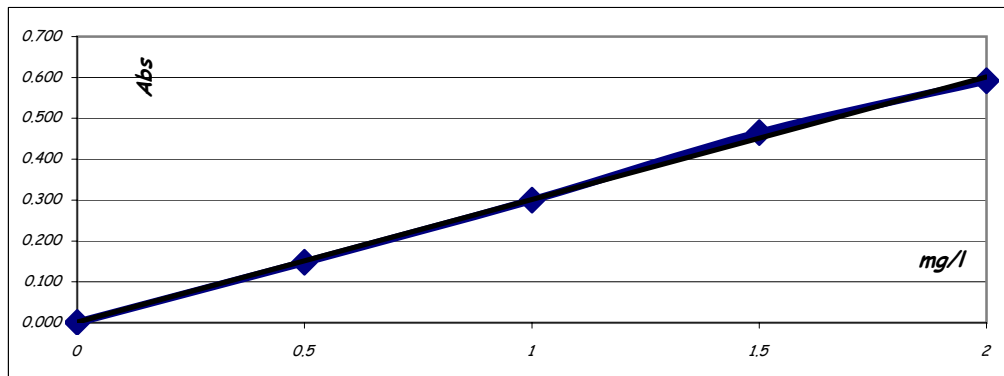

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.300	0.260 to 0.320	Pass
Regression	0.999	0.990 to 1.001	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility

*Tom Russell.*  
 \_\_\_\_\_  
 Dr. T. Russell



An ISO 9001:2008 Registered Company

Annacotty Business Park, Annacotty, Limerick, Ireland.  
 Telephone 061 358190 Facsimile 061 358191