

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      **KR 109**  
**Lot Number**        **1173**

**Date**      06.07.2011


**Expiry Date**      05.07.2012

Reagent	Lot Number
AMM 1	1113
<b>Amn 2</b>	<b>1173</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0.00		0.021
0.25	AMM 10 07 11	0.223
0.50	AMM 10 07 11	0.438
0.77	AMM 10 07 11	0.672
1.00	AMM 10 07 11	0.853


*\*serial dilution*

#### Calibration Curve

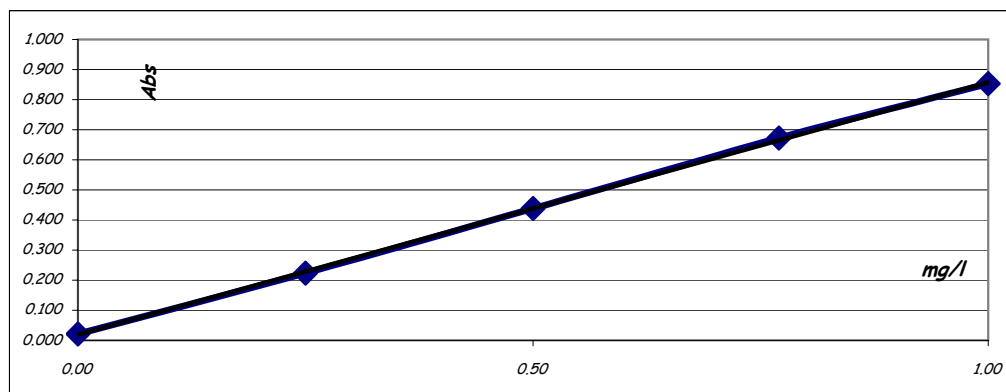

Test	Result	Specification	Pass / Fail
Intercept	0.0187	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.8387	0.750 to 0.890	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

*Notes*      *Store between 2 & 8 °c*  
*\*Stable on Board 5 days*  
*Barcode ID = 109*  
*\* Based on results obtained in our Research Facility*


---

*Dr. T. Russell*