

Certificate of Performance

Hard 1

Product Code KR117

Date 07.07.2011


Expiry Date 06.07.2012

| Reagent | Lot Number |
|-----------------|------------|
| Hard 1 | 1174 |
| Hard 2 | 1080 |
| Hard 3 | 1081 |
| Test Instrument | Konelab 20 |
| Serial Number | P4919028 |

| Std. Value | Lot # | Abs. |
|------------|----------------|-------|
| 0.00 | Hard3000 07 11 | 2.301 |
| 60.00 | Hard3000 07 11 | 2.145 |
| 120.00 | Hard3000 07 11 | 1.941 |
| 181.82 | Hard3000 07 11 | 1.718 |
| 240.00 | Hard3000 07 11 | 1.499 |
| 300.00 | Hard3000 07 11 | 1.268 |

*serial dilution

Calibration Curve

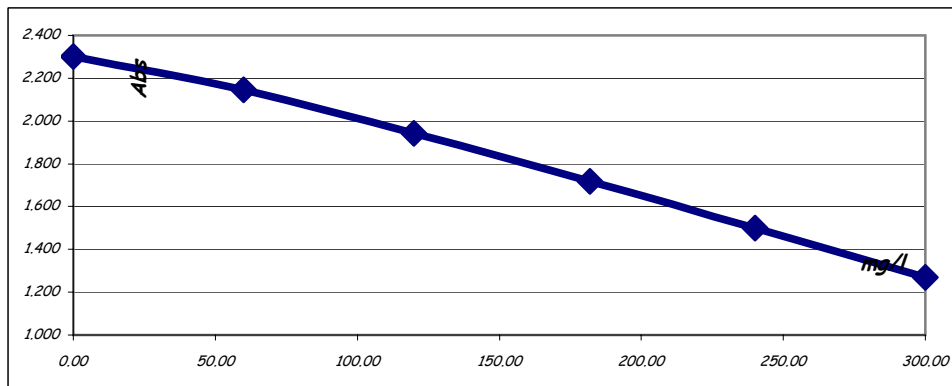

| Test | Result | Specification | Pass/Fail |
|-------------------|---------|--------------------|-----------|
| Sensitivity | | | |
| 0 - 60 mg/l | -0.0026 | -0.0025 to -0.0035 | Pass |
| 60 - 120 mg/l | -0.0034 | -0.0030 to -0.0045 | Pass |
| 120 - 181.82 mg/l | -0.0037 | -0.0035 to -0.0045 | Pass |
| 181.82 - 240 mg/l | -0.0037 | -0.0030 to -0.0040 | Pass |
| 240 - 300 mg/l | -0.0039 | -0.0025 to -0.0040 | Pass |

Notes Store between 2 & 8 °C

Keep Tightly Sealed when not in use.
 Do not return unused portions to container
 Barcode ID- Hard 1 117; Hard 2 118; Hard 3 119
 * Based on results obtained in our Research Facility



Dr. T. Russell