

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **1213**

Date 07.09.2011


Expiry Date 01.09.2012

Reagent	Lot Number
AMM 1	1163
Amm 2	1213
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.029
0.25	AMM 10 07 11	0.220
0.50	AMM 10 07 11	0.429
0.77	AMM 10 07 11	0.658
1.00	AMM 10 07 11	0.860

**serial dilution*

Calibration Curve

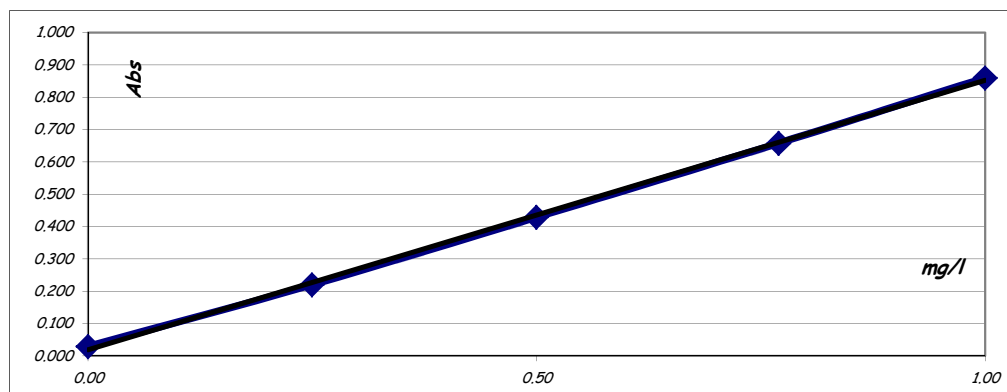

Test	Result	Specification	Pass / Fail
Intercept	0.0192	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8332	0.750 to 0.890	Pass
Regression	0.9994	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*
**Stable on Board 5 days*
Barcode ID = 109
** Based on results obtained in our Research Facility*



Dr. T. Russell