

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR 109**
Lot Number **1225**

Date 21.09.2011


Expiry Date 21.09.2012

Reagent	Lot Number
AMM 1	1189
Amn 2	1225
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.029
0.25	AMM 10 09 11	0.225
0.50	AMM 10 09 11	0.442
0.77	AMM 10 09 11	0.669
1.00	AMM 10 09 11	0.856

**serial dilution*

Calibration Curve

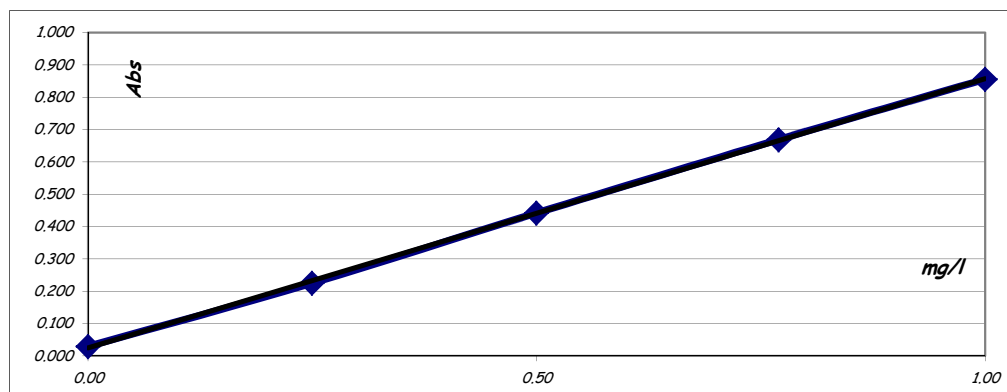

Test	Result	Specification	Pass / Fail
Intercept	0.0245	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8326	0.750 to 0.890	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °c*

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell