

Certificate of Performance
Sulphate Reagent

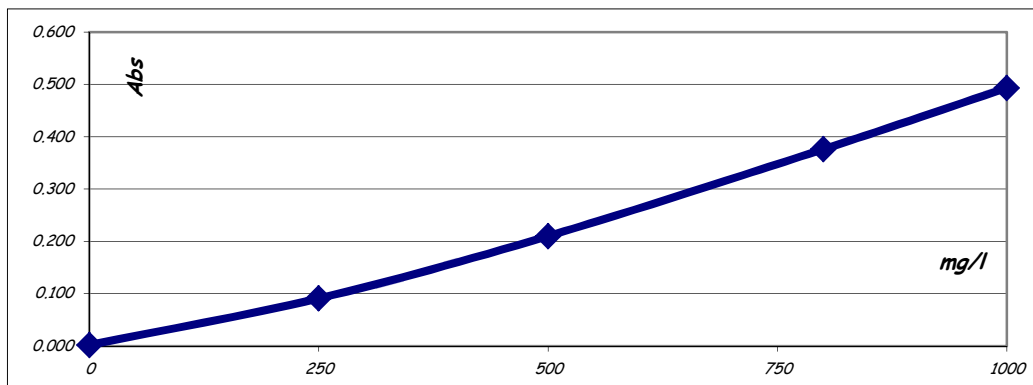
Product Code KR102
Lot Number 1254

Date 25.10.2011 **Expiry Date** 12.10.2012

Reagent	Lot Number
Sulphate	1254
Test Method	LTP01
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.002
250	Sulp 4000 02 11	0.091
500	Sulp 4000 02 11	0.210
800	Sulp 4000 02 11	0.376
1000	Sulp 4000 02 11	0.493

*serial Dilution

Calibration Curve


Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.010	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0004	0.0003 to 0.0006	Pass
250 - 500 mg/l	0.0005	0.0003 to 0.0007	Pass
500 - 800 mg/l	0.0006	0.0004 to 0.0007	Pass
800 - 1000 mg/l	0.0006	0.0004 to 0.0008	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 102
 * Based on results obtained in our Research Facility



Dr. T. Russell