

Certificate of Performance
Ammonia 1 Reagent

Product Code KR108
Lot Number 1255

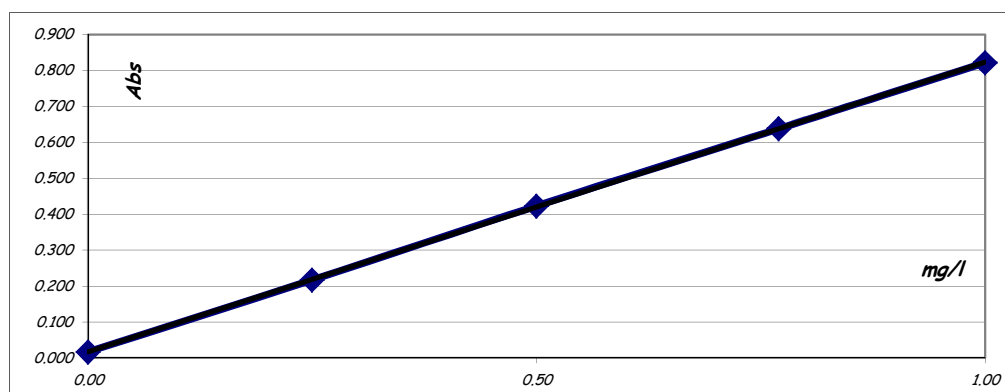
Date 22.11.2011

Expiry Date 12.10.2012

Reagent	Lot Number
AMM 1	1255
Amm 2	1213
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0.00		0.017
0.25	AMM 10 11 11	0.217
0.50	AMM 10 11 11	0.423
0.77	AMM 10 11 11	0.638
1.00	AMM 10 11 11	0.822

**serial dilution*

Calibration Curve


Test	Result	Specification	Pass / Fail
Intercept	0.0172	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.8060	0.750 to 0.890	Pass
Regression	1.0000	0.990 to 1.0001	Pass

Notes Store between 2 & 8 °C

*Stable on Board 1 day

Barcode ID = 108

* Based on results obtained in our Research Facility



Dr. T. Russell