

Certificate of Performance

Chloride Reagent

Product Code KR101
Lot Number 1277


Date 17.11.2011 **Expiry Date** 08.11.2012

Reagent	Lot Number
Chloride	1277
Test Method	LTP02
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.006
250 ppm	CL4000 02 11	0.318
500 ppm	CL4000 02 11	0.515
800 ppm	CL4000 02 11	0.683
1000 ppm	CL4000 02 11	0.777

*serial Dilution

Calibration Curve

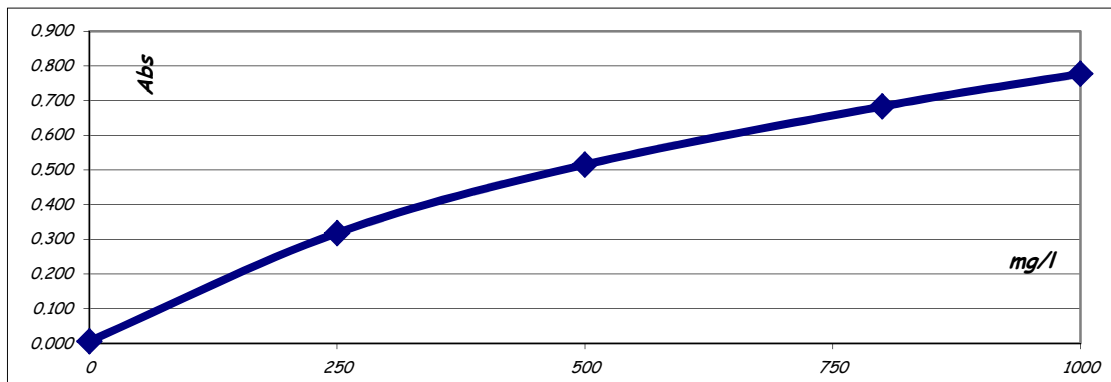

Test	Result	Specification	Pass / Fail
Intercept	0.006	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 250 mg/l	0.0012	0.0010 to 0.0016	Pass
250 - 500 mg/l	0.0008	0.0006 to 0.0012	Pass
500 - 800 mg/l	0.0006	0.0004 to 0.0010	Pass
800 - 1000 mg/l	0.0005	0.0003 to 0.0008	Pass

Notes *Store between 2 & 8 °c*
 **Stable on Board 5 days*
 Barcode ID = 101
 ** Based on results obtained in our Research Facility*

Tom Russell

Dr. T. Russell