

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107
 Lot Number 5013


Date 27.01.2005

Expiry Date 07.08.2005

Reagent	Lot Number
Phos 1	5012
Phos 2	5013
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P0.5 349 04	0.140
1	P1.0 349 04	0.287
1.5	P1.5 349 04	0.430
2	P2.0 349 04	0.570

Calibration Curve

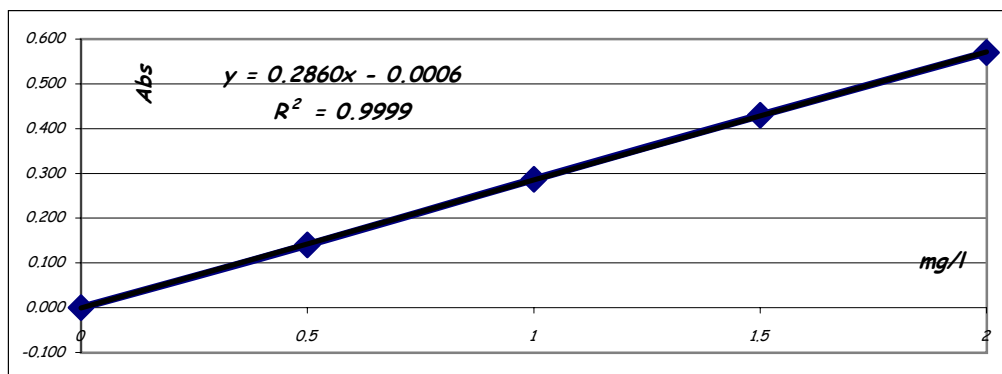

Test	Result	Specification	Pass / Fail
Intercept	-0.001	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.286	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 107
 * Based on results obtained in our Research Facility



Dr. T. Russell