

Certificate of Performance

TON 2 Reagent

Product Code KR 104
Lot Number 5038


Date 09.03.2005

Expiry Date 26.09.2005

Reagent	Lot Number
TON 1	5037
TON 2	5038
TON 3	5039
Test Method	LMTPO3
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.004
2.5	TON2.5 038 05	0.178
5	TON5.0 038 05	0.346
7.5	TON7.5 038 05	0.503
10	TON10 038 05	0.648

Calibration Curve

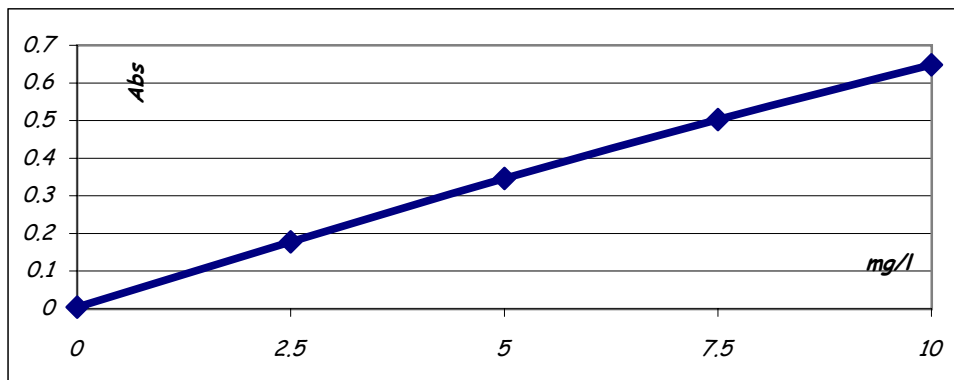

Test	Result	Specification	Pass / Fail
Intercept	0.004	-0.005 to 0.01	Pass
Sensitivity			
Abs/ppm			
0 - 2.5 mg/l	0.0071	0.0055 to 0.0080	Pass
2.5 - 5.0 mg/l	0.0067	0.0060 to 0.0080	Pass
5.0 - 7.5 mg/l	0.0063	0.0050 to 0.0075	Pass
7.5 - 10.0 mg/l	0.0058	0.0050 to 0.0070	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 104
* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell