

Certificate of Performance

TON 2 Reagent

Product Code KR 104
Lot Number 5066


Date 23.05.2005

Expiry Date 23.05.2006

Reagent	Lot Number
TON 1	5065
TON 2	5066
TON 3	5067
Test Method	LMTPO3
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.001
2.5	TON2.5 108 05	0.177
5	TON5.0 108 05	0.345
7.5	TON7.5 108 05	0.499
10	TON10 108 05	0.630

Calibration Curve

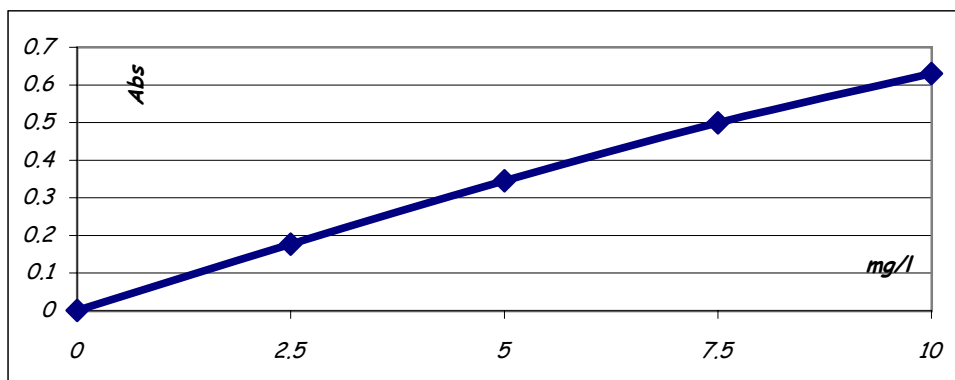

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.5 mg/l	0.0071	0.0055 to 0.0080	Pass
2.5 - 5.0 mg/l	0.0067	0.0060 to 0.0080	Pass
5.0 - 7.5 mg/l	0.0062	0.0050 to 0.0075	Pass
7.5 - 10.0 mg/l	0.0052	0.0050 to 0.0070	Pass

Notes Store between 2 & 8 °C
*Stable on Board 5 days
Barcode ID = 104
* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell