

### Certificate of Performance

#### Phosphate 2 (Phos 2) Reagent

Product Code KR107  
 Lot Number 5069


Date 23.05.2005

Expiry Date 23.05.2006

| Reagent         | Lot Number |
|-----------------|------------|
| Phos 1          | 5068       |
| Phos 2          | 5069       |
| Test Method     | LTP 05     |
| Test Instrument | Konelab 20 |
| Serial Number   | P4919028   |

| Standard Value | Lot #       | Abs.  |
|----------------|-------------|-------|
| 0              |             | 0.000 |
| 0.5            | P0.5 108 05 | 0.144 |
| 1              | P1.0 108 05 | 0.293 |
| 1.5            | P1.5 108 05 | 0.439 |
| 2              | P2.0 108 05 | 0.579 |

#### Calibration Curve

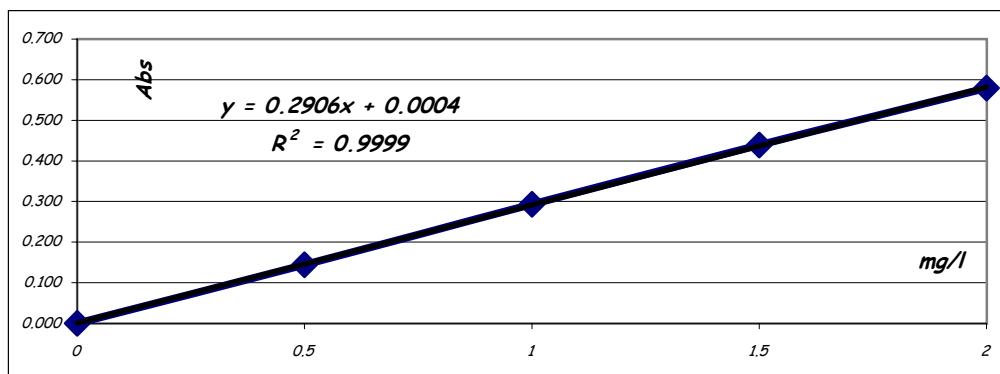

| Test                | Result | Specification   | Pass / Fail |
|---------------------|--------|-----------------|-------------|
| Intercept           | 0.000  | -0.005 to 0.010 | Pass        |
| Sensitivity Abs/ppm | 0.291  | 0.260 to 0.320  | Pass        |
| Regression          | 1.000  | 0.990 to 1.001  | Pass        |

Notes Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 107  
 \* Based on results obtained in our Research Facility



Dr. T. Russell