

## Certificate of Performance

### TON 2 Reagent

Product Code **KR 104**  
Lot Number **5095**


Date **21.07.2005**

Expiry Date **14.07.2006**

Reagent	Lot Number
TON 1	5094
TON 2	<b>5095</b>
TON 3	5096
Test Method	LMTPO3
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.005
2.5	TON2.5 108 05	0.175
5	TON5.0 108 05	0.342
7.5	TON7.5 108 05	0.503
10	TON10 108 05	0.635

### Calibration Curve

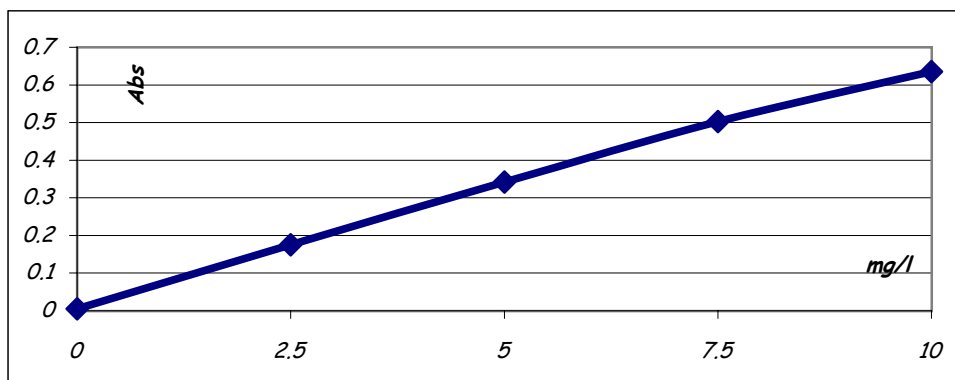

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	<b>Pass</b>
Sensitivity			
Abs/ppm			
0 - 2.5 mg/l	0.0070	0.0055 to 0.0080	<b>Pass</b>
2.5 - 5.0 mg/l	0.0067	0.0060 to 0.0080	<b>Pass</b>
5.0 - 7.5 mg/l	0.0064	0.0050 to 0.0075	<b>Pass</b>
7.5 - 10.0 mg/l	0.0053	0.0050 to 0.0070	<b>Pass</b>

Notes *Store between 2 & 8 °C*  
*\*Stable on Board 5 days*  
*Barcode ID = 104*  
*\* Based on results obtained in our Research Facility*

*Tom Russell.*

Dr. T. Russell