

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107

Lot Number 5098


Date 18.07.2005

Expiry Date 14.07.2006

Reagent	Lot Number
Phos 1	5097
Phos 2	5098
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P0.5 108 05	0.148
1	P1.0 108 05	0.300
1.5	P1.5 108 05	0.442
2	P2.0 108 05	0.580

Calibration Curve

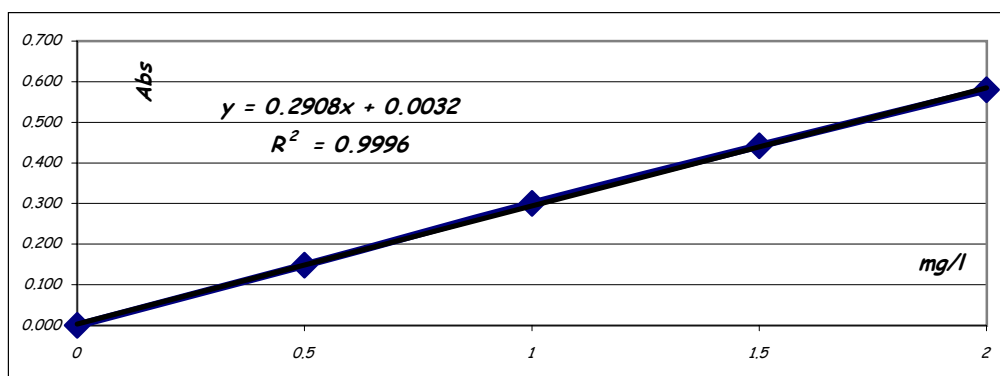

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.291	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 107
 * Based on results obtained in our Research Facility



Dr. T. Russell