

**Certificate of Performance**

**TON 2 Reagent**

**Product Code** KR 104  
**Lot Number** 5139


**Date** 19.10.2005

**Expiry Date** 15.10.2006

Reagent	Lot Number
TON 1	5138
TON 2	5139
TON 3	5140
<b>Test Method</b>	LMTPO3
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0		0.003
2.5	TON2.5 223 05	0.173
5	TON5.0 223 05	0.333
7.5	TON7.5 223 05	0.482
10	TON10 223 05	0.633

**Calibration Curve**

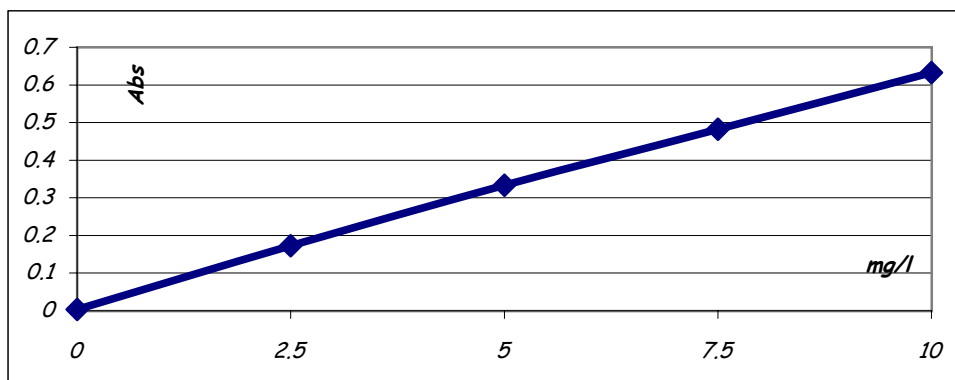

Test	Result	Specification	Pass / Fail
Intercept	0.003	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 2.5 mg/l	0.0069	0.0055 to 0.0080	Pass
2.5 - 5.0 mg/l	0.0064	0.0060 to 0.0080	Pass
5.0 - 7.5 mg/l	0.0060	0.0050 to 0.0075	Pass
7.5 - 10.0 mg/l	0.0060	0.0050 to 0.0070	Pass

**Notes** Store between 2 & 8 °C  
\*Stable on Board 5 days  
Barcode ID = 104  
\* Based on results obtained in our Research Facility

*Tom Russell.*  
\_\_\_\_\_  
Dr. T. Russell