

Certificate of Performance

Phosphate 2 (Phos 2) Reagent

Product Code KR107

Lot Number 5170


Date 06.12.2005

Expiry Date 05.12.2006

Reagent	Lot Number
Phos 1	5169
Phos 2	5170
Test Method	LTP 05
Test Instrument	Konelab 20
Serial Number	P4919028

Standard Value	Lot #	Abs.
0		0.000
0.5	P0.5 332 05	0.144
1	P1.0 332 05	0.285
1.5	P1.5 332 05	0.423
2	P2.0 332 05	0.569

Calibration Curve

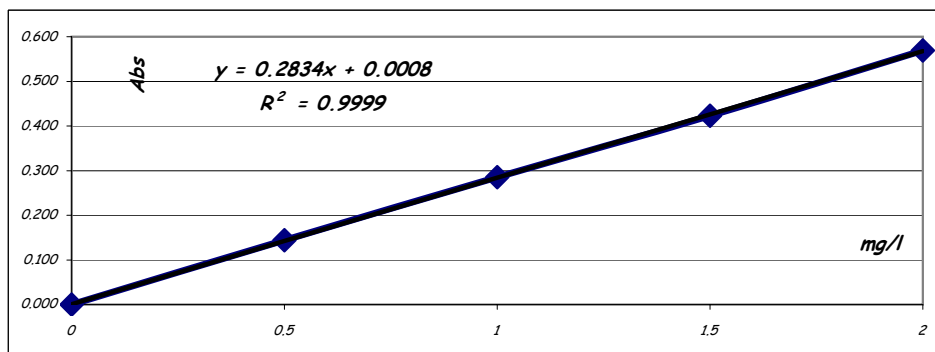

Test	Result	Specification	Pass / Fail
Intercept	0.001	-0.005 to 0.010	Pass
Sensitivity Abs/ppm	0.283	0.260 to 0.320	Pass
Regression	1.000	0.990 to 1.001	Pass

Notes Store between 2 & 8 °C
 *Stable on Board 5 days
 Barcode ID = 107
 * Based on results obtained in our Research Facility

Tom Russell
 Dr. T. Russell