

### Certificate of Performance

#### Ammonia 2 Reagent

**Product Code**      KR109  
**Lot Number**        6002


**Date**      10.01.2006

**Expiry Date**      10.01.2007

Reagent	Lot Number
AMM 1	6001
<b>AMM 2</b>	<b>6002</b>
<b>Test Method</b>	LTP06
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0		0.020
0.25	AM0.25 332 05	0.211
0.5	AM0.5 332 05	0.413
0.8	AM0.8 332 05	0.660
1	AM1.0 332 05	0.815

#### Calibration Curve

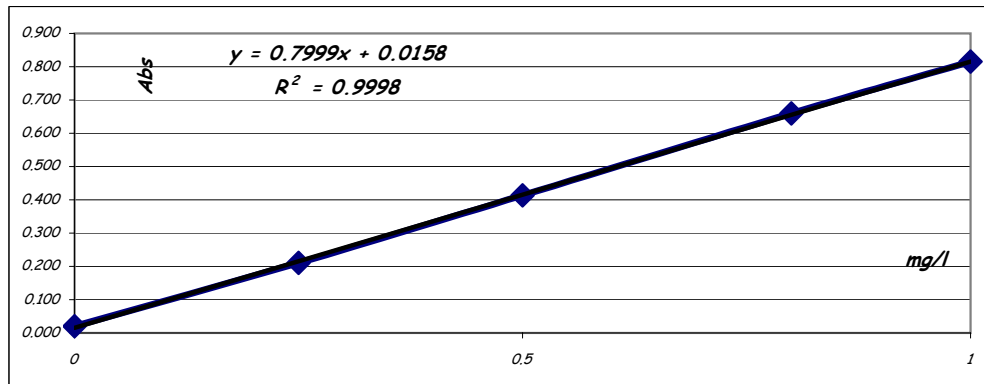

Test	Result	Specification	Pass / Fail
Intercept	0.0158	0.000 to 0.025	<b>Pass</b>
Sensitivity Abs/ppm	0.7999	0.750 to 0.900	<b>Pass</b>
Regression	0.9998	0.990 to 1.0001	<b>Pass</b>

**Notes**      *Store between 2 & 8 °C*

*\*Stable on Board 5 days*

*Barcode ID = 109*

*\* Based on results obtained in our Research Facility*



*Dr. T. Russell*