

Certificate of Performance

Ammonia 2 Reagent

Product Code KR109
Lot Number 6026


Date 20.01.2006

Expiry Date 19.01.2007

Reagent	Lot Number
AMM 1	6025
AMM 2	6026
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.017
0.25	AM0.25 332 05	0.208
0.5	AM0.5 332 05	0.414
0.8	AM0.8 332 05	0.657
1	AM1.0 332 05	0.812

Calibration Curve

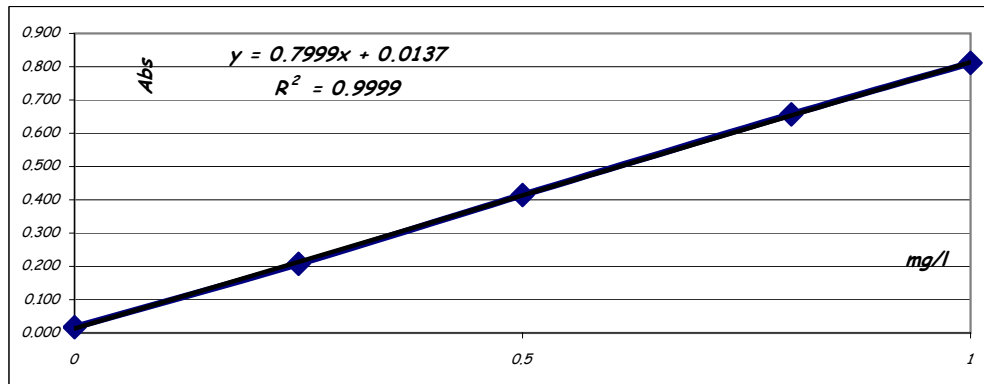

Test	Result	Specification	Pass / Fail
Intercept	0.0137	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7999	0.750 to 0.900	Pass
Regression	0.9999	0.990 to 1.0001	Pass

Notes Store between 2 & 8 °C

*Stable on Board 5 days

Barcode ID = 109

* Based on results obtained in our Research Facility

Tom Russell.

Dr. T. Russell