

'Ready To Use Reagents'



**Certificate of Performance**

**Chloride Reagent**


**Product Code** KR101  
**Lot Number** 6051

**Date** 08.03.2006 **Expiry Date** 02.03.2007

<b>Reagent</b>	<b>Lot Number</b>
Chloride	6051
<b>Test Method</b>	LTP02
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Standard Value	Lot #	Absorbance
0 ppm		0.005
25 ppm	CL25 332 05	0.311
50 ppm	CL50 332 05	0.577
75 ppm	CL75 332 05	0.782
100 ppm	CL100 332 05	0.963

**Calibration Curve**

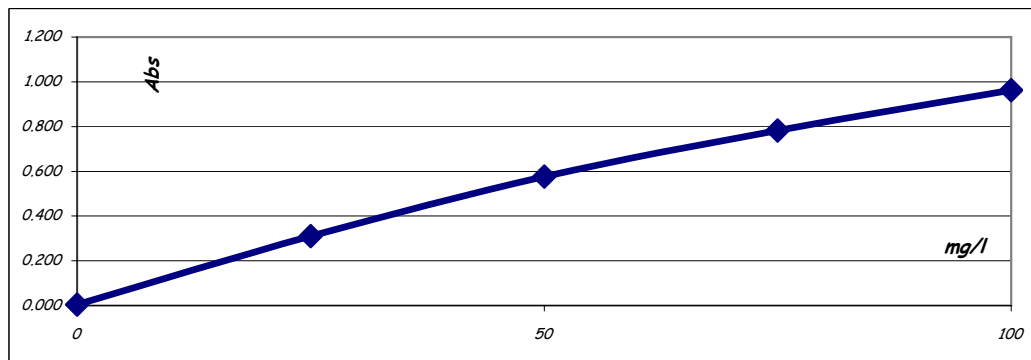

Test	Result	Specification	Pass / Fail
Intercept	0.005	-0.005 to 0.01	Pass
Sensitivity Abs/ppm			
0 - 25 mg/l	0.012	0.0100 to 0.0140	Pass
25 - 50 mg/l	0.011	0.0080 to 0.0120	Pass
50 - 75 mg/l	0.008	0.0065 to 0.0095	Pass
75 - 100 mg/l	0.007	0.0050 to 0.0080	Pass

**Notes** Store between 2 & 8 °C  
 \*Stable on Board 5 days  
 Barcode ID = 101  
 \* Based on results obtained in our Research Facility

*Tom Russell*

Dr. T. Russell