

Certificate of Performance

Ammonia 2 Reagent

Product Code **KR109**

Lot Number **6053**


Date 03.03.2006

Expiry Date 02.03.2007

Reagent	Lot Number
AMM 1	6052
AMM 2	6053
Test Method	LTP06
Test Instrument	Konelab 20
Serial Number	P4919028

Std. Value	Lot #	Abs.
0		0.020
0.25	AM0.25 332 05	0.223
0.5	AM0.5 332 05	0.427
0.8	AM0.8 332 05	0.666
1	AM1.0 332 05	0.816

Calibration Curve

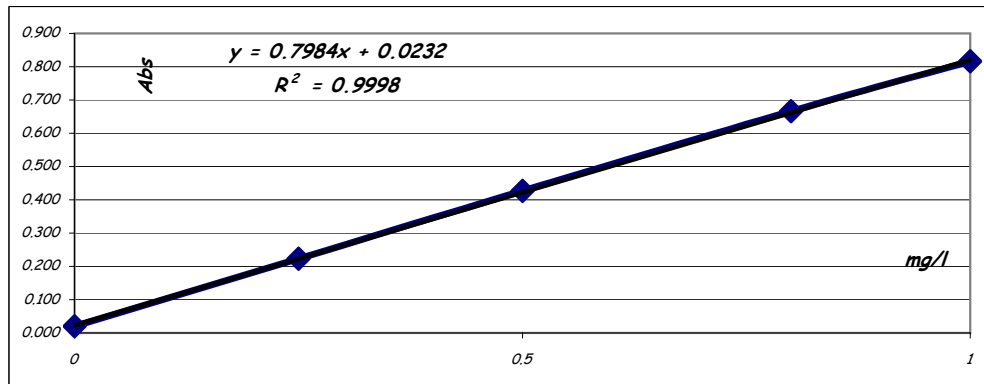

Test	Result	Specification	Pass / Fail
Intercept	0.0232	0.000 to 0.025	Pass
Sensitivity Abs/ppm	0.7984	0.750 to 0.900	Pass
Regression	0.9998	0.990 to 1.0001	Pass

Notes *Store between 2 & 8 °C*

**Stable on Board 5 days*

Barcode ID = 109

** Based on results obtained in our Research Facility*



Dr. T. Russell