

**Certificate of Performance**

**TON 2 Reagent**

**Product Code** KR 104  
**Lot Number** 6060


**Date** 16.03.2006

**Expiry Date** 14.03.2007

Reagent	Lot Number
TON 1	6059
TON 2	6060
TON 3	6061
<b>Test Method</b>	LMTPO3
<b>Test Instrument</b>	Konelab 20
<b>Serial Number</b>	P4919028

Std. Value	Lot #	Abs.
0		0.002
2.5	TON2.5 332 05	0.169
5	TON5.0 332 05	0.330
7.5	TON7.5 332 05	0.482
10	TON10 332 05	0.616

**Calibration Curve**

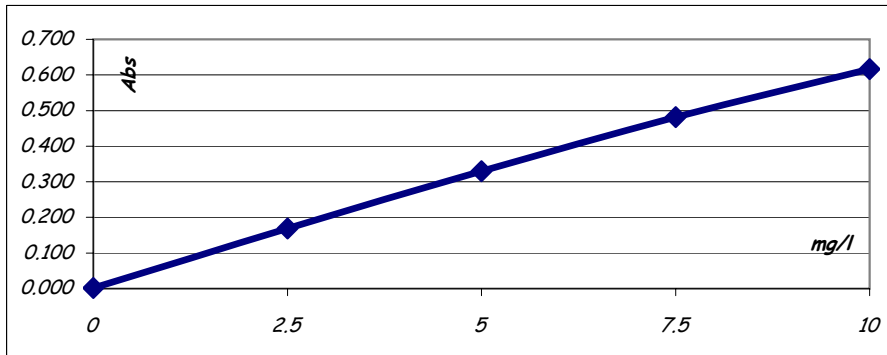

Test	Result	Specification	Pass / Fail
Intercept	0.002	-0.005 to 0.01	<b>Pass</b>
Sensitivity Abs/ppm			
0 - 2.5 mg/l	0.0068	0.0055 to 0.0080	<b>Pass</b>
2.5 - 5.0 mg/l	0.0064	0.0060 to 0.0080	<b>Pass</b>
5.0 - 7.5 mg/l	0.0061	0.0050 to 0.0075	<b>Pass</b>
7.5 - 10.0 mg/l	0.0054	0.0050 to 0.0070	<b>Pass</b>

**Notes** Store between 2 & 8 °c  
\*Stable on Board 5 days  
Barcode ID = 104  
\* Based on results obtained in our Research Facility

*Tom Russell.*

Dr. T. Russell